



Citation for published version:

Biguri, A & Soleimani, M 2015, 'Statistical and deterministic approaches for electrode movement in lung EIT', Paper presented at EIT2015, Swaziland, 1/06/15 - 5/06/15.

Publication date:
2015

Document Version
Early version, also known as pre-print

[Link to publication](#)

Each individual paper in the collection (C) 2015 by the indicated authors.

University of Bath

Alternative formats

If you require this document in an alternative format, please contact:
openaccess@bath.ac.uk

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Statistical and deterministic approaches for electrode movement in lung EIT

Ander Biguri and Manuchehr Soleimani

Engineering Tomography Lab (ETL), Electronic and Electrical Engineering, University of Bath, Bath, UK,
a.biguri@bath.ac.uk

Abstract: Electrode movement can be a challenging issue in EIT modelling. In cases where the imaged region is changing, such as lung EIT, small artefacts may arise. To cope with this artefacts some deterministic and statistic approaches are available in the literature. In this work both are compared against expected electrode movement in lung EIT imaging.

1 Introduction

In lung EIT monitoring electrodes will slightly move from their position due to breathing. The mismatch between the simulated model and the real geometry of the patient can lead to some artefacts in image reconstruction. To account for the electrode movement a deterministic approach using an extended Jacobian and a statistical approach using approximation error models is available in the literature [1] [2]. The objective of the study is to compare both approaches in a realistic scenario.

2 Methods

2.1 Reconstruction algorithms

The inverse problem solution is expressed using an statistical approach as the Maximum A Posteriori (MAP). The error between the measured voltage V and approximated voltage (by the known model) $U_h(\sigma, \tilde{\gamma})$ (where σ is conductivity and $\tilde{\gamma}$ approximated boundary condition) is defined as η . If the prior and noise covariance matrix are defined as Γ_σ and $\Gamma_{\eta|\sigma}$ respectively and their Cholesky factors are L_σ and $L_{\eta|\sigma}$. The solution of the most likely conductivity values that maximizes the posterior distribution is described as

$$\sigma_{MAP} = \arg \min_{\sigma} \left\{ \left\| L_{\eta|\sigma} (V - U_h(\sigma, \tilde{\gamma}) - \eta_{*|\sigma}) \right\|^2 + \left\| L_{\sigma} (\sigma - \sigma_*) \right\|^2 \right\}. \quad (1)$$

This specific MAP description is generally refereed as MAP with approximation error model (MAP-AEM), as it includes the errors that are present in the system as noise.

The statistical approach to deal with predictable errors is to model the expected noise mean and standard deviation off-line[1]. Alternatively, an extended sensitivity matrix can be built in order to have a deterministic linear approximation of the movement of the electrodes with respect to the measured voltages [2].

2.2 Simulations

To compare the results, the electrode movement created by human breathing is simulated[3]. Additionally statistical modelling of standard deviation and mean of the noise are preformed. Then image reconstruction using the statistical and deterministic approach is performed.

2.2.1 Results

To evaluate the quality of the resulting images some performance figures are used, modified from the GREIT parameters [4] and image processing literature [5]. The robustness is the evaluated property in this work, therefore the coefficient of variation of the parameters for the whole breathing cycle is calculated, as in table 1.

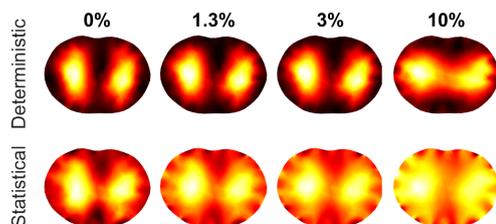


Figure 1: Deterministic (top) and statistical (bottom) approaches against amount of electrode movement in breathing. Movement of 0%, 1.5%, 3% and 10% o the boundary size.

3 Conclusions

This paper compares the statistical and deterministic approaches for electrode movement due to breathing. The AEM seems to have worse performance in general. A critical evaluation of AEM based method and deterministic method will be presented.

4 Acknowledgements

This work is funded by a EPSRC DTA and CERN.

References

- [1] Kaipio JP, Kolehmainen V, Somersalo E, et al. *Inverse Problems* **16**(5):1487, 2000
- [2] Soleimani M, Gómez-Laberge C, Adler A. *Physiol Meas* **27**(5):S103, 2006
- [3] Zhang J, Qin L, Allen T, et al. *Open Biomed Eng J* **15**(7):109–15, 2013
- [4] Adler A, Arnold J, Bayford R, et al. *Physiol Meas* **30**(6):S35, 2009
- [5] Burger W, Burge MJ. *Principles of Digital Image Processing, Fundamental techniques*. Springer, 2009

Table 1: Mean and standard deviation of the coefficient of variation in performance figures of statistical and deterministic method.

	TA	RES	SD	RNG	Corr.	Mutual info.	Sharp.
Determ.	$12.6e^{-3} \pm 1.5e^{-3}$	$11.6e^{-3} \pm 1.6e^{-3}$	1.16 ± 0.11	0.26 ± 0.03	$16.1e^{-3} \pm 1.7e^{-3}$	$4.9e^{-3} \pm 0.5 e^{-3}$	$21.5e^{-3} \pm 2.8e^{-3}$
MAP-AEM	0.1 ± 0.01	$43e^{-3} \pm 7.6e^{-3}$	0.8 ± 0.2	0.42 ± 0.06	0.19 ± 0.02	0.12 ± 0.01	0.33 ± 0.049